

[REDACTED]

DEKRA Testing and Certification GmbH
Standort Essen
Persönliche Schutzausrüstungen

Adlerstraße 29
45307 Essen, Germany

Tel [REDACTED]
Fax [REDACTED]
E-Mail DTC-Support-Essen@dekra.com

Prüfbericht / Test report

[REDACTED]


Prüfgegenstand <i>Testsubject</i>	Corona SARS-CoV-2 Atemschutzmaske <i>Corona SARS-CoV-2 respiratory protective mask</i>
Modell <i>Type</i>	[REDACTED] [REDACTED]
Hersteller <i>Manufacturer</i>	Ningbo Troika Science & Technology Co. Ltd. 11 Gaoya Rd, Jiangshan Town Ningbo China
Prüfgrundlage <i>Test requirement</i>	Prüfgrundsatz für Corona SARS-Cov-2 Pandemie Atemschutzmasken Rev. 1 vom 26.03.2020 <i>Testing principle for Corona SARS-CoV-2 pandemic respiratory masks rev. 1 of 2020-03-26</i>
Prüfergebnis <i>Test result</i>	Die Pandemie Atemschutzmaske entspricht der Corona SARS-CoV-2 Prüfanforderung <i>The pandemic respiratory protective mask does meet the Corona SARS- CoV-2 test requirement.</i>
Datum <i>Date of issue</i>	07.04.2020

Dieser Bericht besteht aus 11 Seiten. *This report consists of 11 pages.*

Eine auszugsweise Veröffentlichung dieses Berichtes bedarf der Zustimmung der DEKRA Testing and Certification GmbH. Juristisch bindend ist ausschließlich die deutsche Fassung dieses Berichtes.

Publication of extracts of this report requires agreement of DEKRA Testing and Certification GmbH. We confirm the correctness of the translation of the German original. In the case of arbitration however only the German wording shall be valid and binding.



DEKRA Testing and Certification GmbH, Handwerkstraße 15, 70565 Stuttgart
Zertifizierungsstelle *Certification Body*: Dinnendahlstraße 9, 44809 Bochum
Telefon [REDACTED] DTC-Certification-body@dekra.com



Veranlassung / Reason

Auftragseingang <i>Date of order</i>	01/04/2020
Auftraggeber <i>Applicant</i>	Imwalle GmbH & Co. KG Lange Str. 78, 49610 Quakenbrück
Importeur <i>Importer</i>	Eifa Warenhandels GmbH Lange Str. 78, 49610 Quakenbrück
Eingang der Prüfmuster <i>Date of receipt of test item</i>	03/04/2020
Prüfzeitraum <i>Date (s) of performance of tests</i>	03/04/2020 – 07/04/2020
Prüfstandort <i>Test location</i>	DEKRA Testing and Certification GmbH Persönliche Schutzausrüstungen Adlerstraße 29 45307 Essen, Germany


Zusammenfassung der Prüfung / Summary of Testing




DEKRA Testing and Certification GmbH




(Dr. Spittle
Prüfingenieur / Test engineer






Inhaltsverzeichnis / Table of contents








1 Bezug der Prüfergebnisse / Reference of the test results





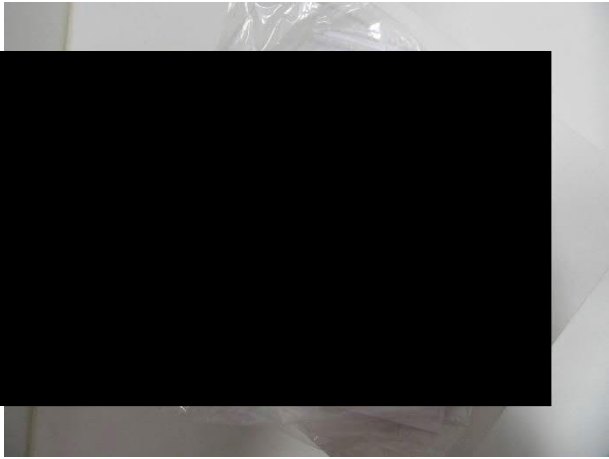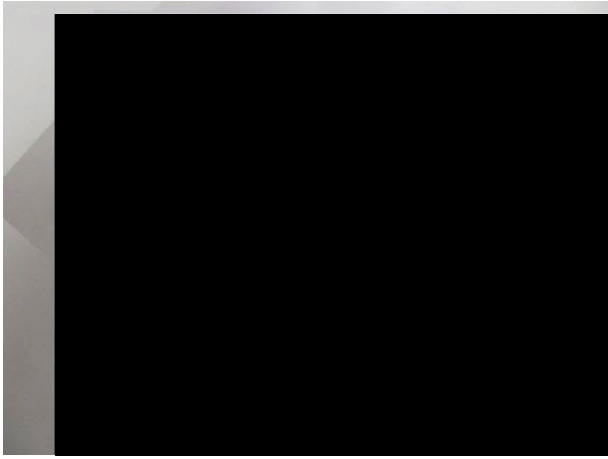
	
Verpackung / Packaging	Verpackung / Packaging
	
Gebrauchsanweisung / User manual	Gebrauchsanweisung / User manual

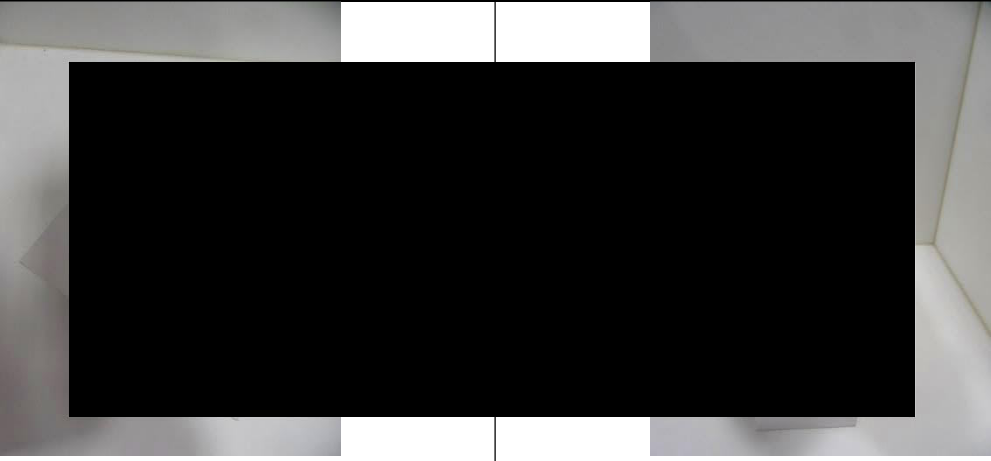


	
Seitenansicht / <i>Side view</i>	Frontansicht / <i>Front view</i>










--	--	--







Certificate to Letter of assessment

in accordance with enactment [REDACTED] as well as according to "Test principle for Corona SARS-Cov-2 pandemic respirators Rev. 0 dated 20.03.2020" for placing on the market in Austria

Issued to distributor

BIO OIL DEVELOPMENT GMBH
Seidlgasse 21/1/10
1030 Wien
Austria

manufacturer

Ningbo Troika Science & Technology Co. Ltd.
11Gaoya Rd
Jiangshan Town Ningbo
P.R. China

Based on the documents submitted and the examinations carried out this is to certify, that the Corona Virus Pandemic Respirator (CPA)

[REDACTED]
(photo documentation see reverse side)

corresponds to the requirements of the shortened assessment process in accordance with enactment GZ 2020 0.198.830 as well as according to "Test principle*) for Corona SARS-Cov-2 pandemic respirators Rev. 0 dated 20.03.2020" for placing on the market in Austria based on EN 149:2001+A1:2009, the following can be stated:

note) The fit of the mask depends on the face shape of the wearer, so a fit check must be carried out before use.
Appropriate information must be enclosed with the mask.

This new PPE will be assigned to **category III**

This letter of assessment applies only to Corona Virus Pandemic Respirator (CPA) to [REDACTED] of the current health threat and / or until the [REDACTED]

Ing. Judith Pointner
Head of Certification Body
OETI - Institute for Ecology, Technology and Innovation; Notified Body No. NB [REDACTED]
Vienna, 08.05.2020

*) non-harmonized standard

"Certificate" Page 1 of 2 Pages
certificate to Letter of assessment [REDACTED]

OETI - Institut für Ökologie, Technik und Innovation GmbH | Spengergasse 20, 1050 Vienna, Austria
[REDACTED] | email office@oeti.at | FN 326826b | VAT No. ATU65149029
www.oeti.at

Member of TESTEX Group



Príloha č. 2 - Návrh na plnenie kritéria na vyhodnotenie ponúk a identifikačné údaje uchádzača

Obchodné meno uchádzača:	TaJaMed s.r.o.
Sídlo uchádzača:	Slnečná 763/1, Malinovo, 90045
IČO:	52631133
Meno a priezvisko štatutárneho zástupcu	Zuzana Beňová
IČ DPH:	SK2121106845
Názov banky:	SLSP
Číslo účtu (IBAN):	
Telefónne číslo:	
E-mailová adresa:	management@tajamed.sk

Predmet zákazky: „Respirátor FFP3 bez výdychového ventilu“

Kritérium na vyhodnotenie ponúk: najnižšia cena za celý predmet zákazky v EUR s DPH.

N á z o v	Celková cena v EUR s DPH
Respirátor FFP3 bez výdychového ventilu v celkovom množstve 20 000 ks v súlade s opisom predmetu zákazky tejto výzvy č. 26	23 800,00

Cena uvedená uchádzačom obsahuje všetky náklady, ktoré uchádzačovi vzniknú v súvislosti s plnením predmetnej zákazky. Verejný obstarávateľ upozorňuje, že novelou 67/2020 Z. z. účinnou od 12.02.2021 sa na respirátory FFP3 a FFP2 zaviedla 0 (nulová) DPH. Na základe uvedeného **bude celková cena s DPH totožná s celkovou cenou bez DPH a to bez ohľadu na to, či uchádzač je alebo nie platiteľom DPH.**

V Malinove, dňa 28.02.2021

meno a priezvisko
podpis štatutárneho zástupcu,
pečiatka